

EXPERIMENTAL APPARATUS FOR SMA ACTUATORS TESTING

Submitted 26th June 2011; accepted 3rd September 2011

Miroslav Dovica, Tatiana Kelemenová, Michal Kelemen

Abstract:

Paper deals with measuring apparatus for shape memory alloy (SMA) wire actuators. The apparatus has been developed as didactic tool for exercises in mechatronic study program. Apparatus enable contact-less measuring of static and dynamic characteristic of SMA actuators.

Keywords: SMA actuator; measuring; mechatronics

1. Introduction

The most famous SMA material is Nitinol, which is an alloy of nickel and titanium. It has been discovered in Naval Ordnance Laboratory in sixty years of twentieth century. Phenomenon of SMA occurs in more than 20 alloy types. The SMA actuators are made as wire, spring or ribbons shape.

Nitinol wire actuator named as FLEXINOL 250LT with 0.25 mm in diameter has been tested in this paper. Recommended activation temperature is 70 °C. Recovery force is recommended at value of 9,3 N. Activation electric current is defined at the 1000 mA. Limit maximum stress (pull force) is 172 MPa [3].

In this paper, the contraction and pull recovery test stand has been developed for testing of SMA wire actuator [1, 2, 3, 4, 5, 6, 7].

2. Apparatus arrangement

Apparatus (Fig. 1, 2) consists of a frame with an arm and two pulleys for guiding of nylon wire connected with SMA wire actuator. One end of the Flexinol wire is attached to the frame and second free end is connected *via* nylon wire with bias weight. Nylon wire is guided with two pulleys to the place for hook with bias weight. There is a reference point (Fig. 3) from permanent magnet placed on the nylon wire. Deformation of the Flexinol wire is represented with the reference point (permanent magnet) and position of the magnet is measured *via* Hall position sensor SS495A. Consequently, output sensor voltage represents the deformation of the Flexinol wire.

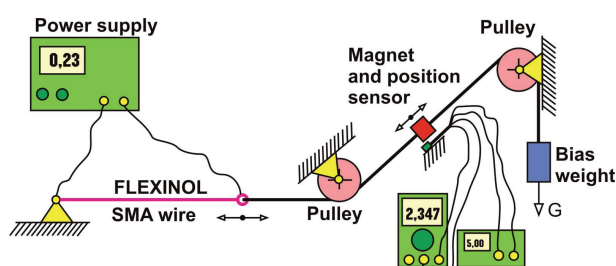


Fig. 1. Measuring apparatus arrangement

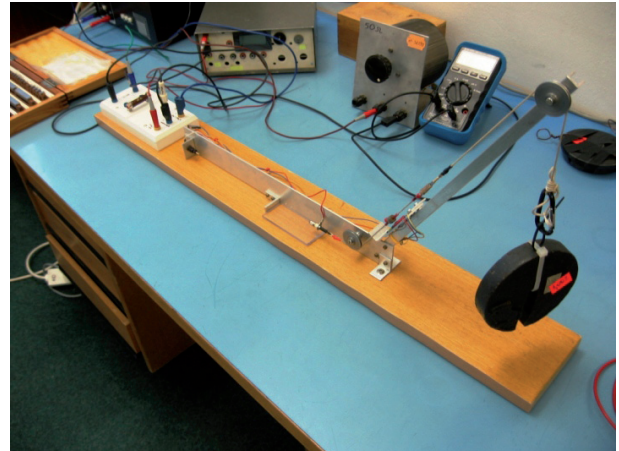


Fig. 2. Realization of SMA actuator measuring apparatus

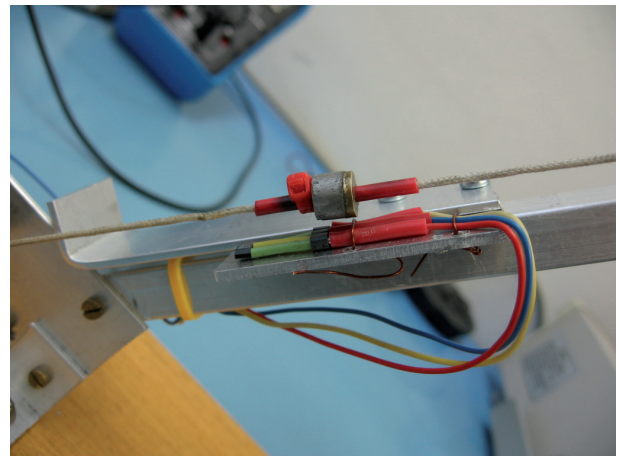


Fig. 3. Reference point (magnet) for contact-less measuring of SMA deformation

It is necessary to do calibration of the hall position sensor with length etalons (Fig. 4). The calibration process associates the sensor output voltage with Flexinol wire deformation.

Results from calibration process are shown in Figure 4. Output sensor voltage has nonlinear behavior which corresponds to Flexinol free end position. The measured points are as result of average from 10 measurements. Expected uncertainty of measurement for measurement of position is 0.2 mm. Uncertainties of length etalons have been neglected. Relation between the free end position and output sensor voltage has been fitted *via* polynomial model mentioned in Figure 5.

Thermal activation of the SMA can be easily driven by electrical current from power supply *via* Joule heating. Cooling of the SMA can be realized *via* heating radiation into surroundings at the room temperature.

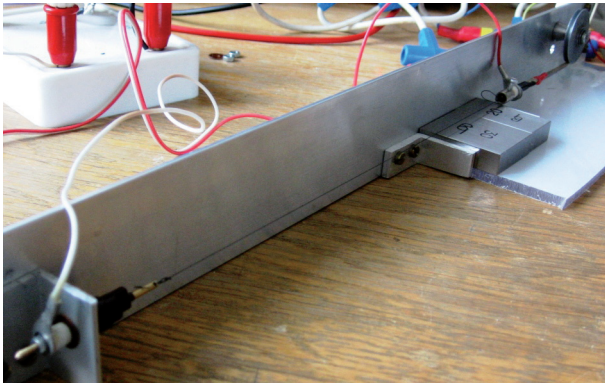


Fig. 4. Calibration process of contact-less measuring of SMA deformation

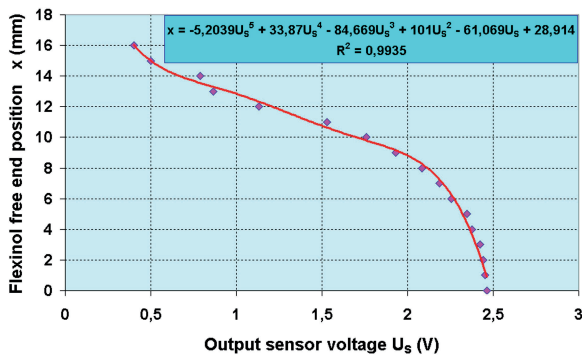


Fig. 5. Calibration process characteristic

Heating and cooling of the Flexinol causes change of the Flexinol free end position. Fig. 6 shows this dependence of free end Flexinol position on value of electric current, which shows highly nonlinearity and hysteresis behavior. The characteristic shown in Fig. 6 has been measured with bias weight 1 kg, which corresponds to maximum recommended pull stress.

Dynamic characteristic has been tested through the step response testing. Excitation electric current is shown in Fig. 7 and it has been controlled *via* microcontroller. Step response has been measured *via* measuring adapter MF624 with personal computer in Matlab/Simulink environment.

The designed test bench also enables to cyclic test life-time of actuator.

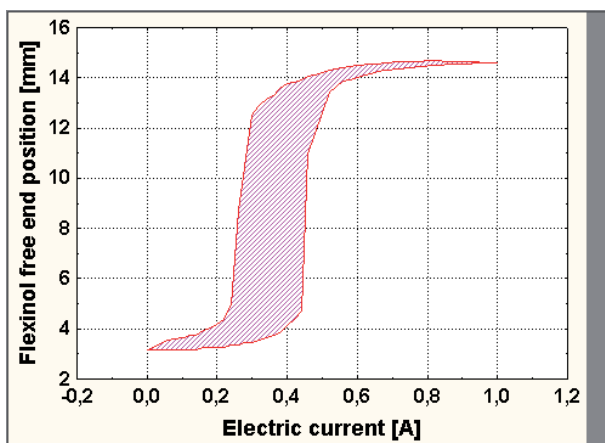


Fig. 6. Static characteristic of SMA wire actuator

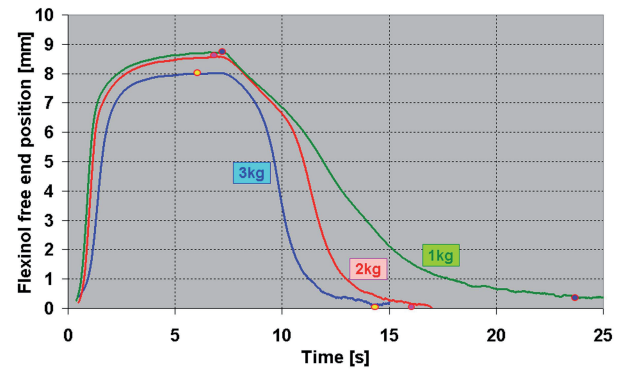
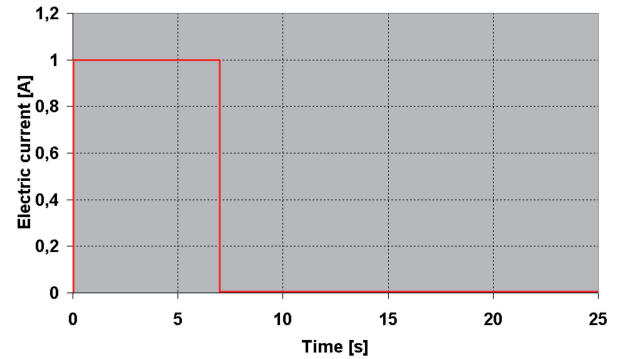


Fig. 7. Actuator step response testing

It is possible to determine activation and deactivation time for Flexinol which are correspond with heating and cooling time. Figure 7 shows that cooling is slower then heating. Step response is tested for overloaded mode and it is possible to say that overloading causes a decreasing of the heating and cooling time. Students also can identify mathematic model of actuator, which can be inserted into complex model of the mechatronic system.

3. Conclusion

The measuring apparatus is used as didactic tool for practical exercises in mechatronic subjects. Students can practically try to use SMA wire actuator. They can test various condition of actuator using.

Shape memory alloy has a lot of advantages as clean, silent and spark free operation, high biocompatibility and excellent corrosion resistance. They are also free of parts such as reduction gears and do not produce dust particles. Actuators based on this principle are very often used in robotic and mechatronic application [8, 9, 10, 11, 12].

Acknowledgements

The authors would like to thank to Slovak Grant Agency – project VEGA 1/0022/10 „A contribution to the research of measuring strategy in coordinate measuring machines”. This contribution is also the result of the project implementation: Centre for research of control of technical, environmental and human risks for permanent development of production and products in mechanical engineering (ITMS:26220120060) supported by the Research & Development Operational Programme funded by the ERDF.

AUTHORS

Miroslav Dovica* – Technical University of Košice, Faculty of Mechanical Engineering, Letná 9, 042 00 Košice, Slovak Republic, e-mail: miroslav.dovica@tuke.sk.

Tatiana Kelemenová – Technical University of Košice, Faculty of Mechanical Engineering, Letná 9, 042 00 Košice, Slovak Republic, e-mail: tatiana.kelemenova@tuke.sk.

Michal Kelemen – Technical University of Košice, Faculty of Mechanical Engineering, Letná 9, 042 00 Košice, Slovak Republic, e-mail: michal.kelemen@tuke.sk.

*Corresponding author

References

- [1] Andrianesis K., Koveos Y., Nikolakopoulos G., and Tzes A., *Experimental Study of a Shape Memory Alloy Actuation System for a Novel Prosthetic Hand*, ed. by: Corneliu Cismasiu, ISBN: 978-953-307-106-0, Publ. InTech, August 2010, pp. 81-105.
- [2] E. M. Severinghaus “Low Current Shape Memory Alloy Devices” U.S. Patent US6969920B1, Nov. 29, 2005. Monodotronics.
- [3] DYNALLOY Inc., Flexinol Technical Characteristics, [online]. Document Version 2011/01/02 T15:31:00Z 2011 [cit. 2011-01-02]. available online: <<http://www.dynalloy.com>>.
- [4] Shik Hoi-yin, “Metal has memmory??”, [online]. Document Version 2011/01/02 T17:45:00Z 2011 [cit. 2011-01-02]. available online: http://www.phy.cuhk.edu.hk/phyworld/iq/memory_alloy/memory_alloy_e.html.
- [5] P. Drahoš, O. Čičáková, “Measurement of SMA Drive Characteristics”, *Measurement Science Review*, vol. 3, section 3, 2003, pp. 151-154.
- [6] ASTM F 2082 – 01 Standard Test Method for Determination of Transformation Temperature of Nickel-Titanium Shape Memory Alloys by Bend and Free Recovery.
- [7] Janke L., Czaderski C., Motavalli M., Ruth J., “Applications of shape memory alloys in civil engineering structures – Overview, limits and new ideas”, *Materials and Structures*, vol. 38, June 2005, pp. 578-592.
- [8] Vitko A., Jurišica L., Kľúčik M., Duchoň F., “Context Based Intelligent Behaviour of Mechatronic Systems”, *Acta Mechanica Slovaca*, vol. 12, 2008, part 3-B, pp. 907-916. ISSN 1335-2393.
- [9] Vitko A., Jurišica L., Kľúčik M., *et al.*, “Embedding Intelligence Into a Mobile Robot”, *AT&P Journal Plus*, no. 1: Mobile robotic systems, 2008, pp. 42-44. ISSN 1336-5010.
- [10] Olasz A., Szabó T., “Direct and inverse kinematical and dynamical analysis of the Fanuc LR Mate 200IC robot”. In: *XXV. International Scientific Conference microCAD*, March-April 2011, p. 37-42.
- [11] Lénárt J., Jakab E., “Machine vision used in robotics”. In: *OGÉT 2010, XVIII. International Conference on Mechanical Engineering*, 2010, p. 272-274. (In Hungarian)
- [12] Antal D., “Dynamical modelling of a path controlled vehicle”. In: *XXIV. Micro CAD, International Scientific Conference*, 2010, pp. 1-6.