

ESTIMATION OF LAYER THICKNESS BY COST FUNCTION OPTIMIZATION: PHANTOM STUDY

**JURIJ TASINKIEWICZ, JERZY PODHAJECKI, JANUSZ WOJCIK,
KATARZYNA FALIŃSKA, JERZY LITNIEWSKI**

Ultrasound Department
Institute of Fundamental Technological Research Polish Academy of Sciences,
Pawińskiego 5b, 02-106 Warszawa, Poland
yurijtas@ippt.pan.pl

The aim of this work is to present the preliminary results of the layer thickness assessment method based on the optimization approach. The developed method is based on a multilayer model structure. The measured acoustic signal reflected from the layer is compared with a simulated signal on the basis of the multilayer model. The cost function is defined as the difference between the reflected signal measured using the pulse echo approach and the simulated signal. The thickness of the solid layer is the parameter which minimizes the cost function yielding the desired solution. Minimization of the cost function is performed with the use of the simulated annealing algorithm. The results obtained with the developed method using the measurement data of a custom design model are compared with the reference value and the accuracy of the method is verified. The relative error of the thickness estimation is 1.44%.

INTRODUCTION

The main objective of this work is to present a noninvasive method of layer thickness assessment. Several methods have been reported which allow the thickness of the layer to be measured using reflected acoustic waves. The envelope [1] or autocorrelation methods [2] can be applied in cases when reflections from layer interfaces are separated over time. For cases in which internal reflections overlap, the reflected signal can be subjected to cepstral analysis [3]. There are, in addition to this, other methods such as the parametric method [4] or the maximum entropy analysis method [5], which allow the thickness of the layer to be determined when the reflected signal consists of interfering components. In this paper we present a new approach of layer thickness estimation based on the cost function optimization scheme. The reported method is based on the analysis of the acoustic wave-field reflected from the multilayered system. More specifically, the liquid – solid layer – porous medium structure is considered here. This method was tested using the measurement data of a custom design model consisting of a solid layer as well as porous material. The proposed method can

be applied for cortical bone thickness assessment using reflected ultrasound, which could be potentially useful information in the diagnosis of osteoporosis.

1. THEORETICAL BACKGROUND

The analyzed multi-layer structure is shown in Fig. 1. Here, a straightforward analysis of acoustic wave propagation may be conducted. The incident wave propagates in the first layer media and impinges upon the second layer at a right angle. In this particular case, only a longitudinal wave exists. It was observed earlier that the temporal spectrum of the ultrasonic pulse reflected from the layered media depends strongly on the thickness of the corresponding layers [3]. This property is used in the further part of the analysis.

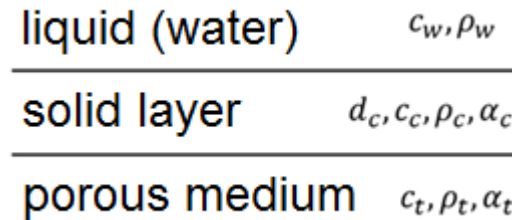


Fig. 1. Multi-layer structure.

In Fig. 1 ρ denotes mass density, c is acoustic wave velocity (a longitudinal wave is assumed), α is the attenuation coefficient; the subscripts w, s, p denote the first, second and third regions (water, solid and porous media), respectively; d_s is the thickness of the solid layer. The acoustic signal of the reflected wave can be modeled using the following formula which results from the linear system approach:

$$\hat{S}^R(\omega, \theta, d_s) = R(\omega, \theta, d_s) S^I(\omega), \quad (1)$$

which gives the dependence between the temporal spectra of the interrogating pulse $S^I(\omega)$ (superscript I denotes the incident wave) and the reflected signal $\hat{S}^R(\omega, \theta, d_s)$ in the layered media, as shown in Fig. 1, which is characterized by the reflection coefficient $R(\omega, \theta, d_s)$. In the Eq. (1) ω is the temporal angular frequency, and θ denotes the parameters of the model (attenuation, acoustic wave velocity, mass density). For the analyzed structure, an analytical solution for the reflection coefficient can be derived as shown in [6]:

$$R = \frac{B_{21} + B_{22}Z_p - (B_{11} + B_{12}Z_p)Z_w}{B_{21} + B_{22}Z_p + (B_{11} + B_{12}Z_p)Z_w}, \quad (2)$$

where the elements of the transmission matrix are given below:

$$B_{11} = B_{22} = \cos k_s d_s; \quad B_{12} = \frac{j}{Z_s} \sin k_s d_s; \quad B_{21} = j Z_s \sin k_s d_s. \quad (3)$$

In the Eq. (3) k_i and $Z_i = \rho_i c_i$, $i = w, s, p$ denote the wave number and acoustic impedance of liquid (water), solid and porous media regions, respectively. The corresponding velocities c_s and c_p in the second and third regions are complex valued functions of ω , due to the attenuation taken into account in the model above. In this case the corresponding wave numbers are defined as follows:

$$k_i \equiv \frac{\omega}{\bar{c}_i} = \frac{\omega}{c_i} - j\alpha_i, \quad i = s, p, \quad (4)$$

The difference between the temporal spectrum of the measured reflected signal and the one obtained from the model presented by Eq. (1) can be defined as follows:

$$e(\omega, \theta, d_s) = S^R(\omega, \theta, d_s) - \hat{S}^R(\omega, \theta, d_s) = S^R(\omega, \theta, d_s) - R(\omega, \theta, d_s)S^I(\omega), \quad (5)$$

where $S^R(\omega, \theta, d_s)$ is the temporal spectrum of the measured reflected signal; $e(\omega, \theta, d_s)$ is the difference between both the measured and modeled spectra. The reflected signal in Eq. (6) is modeled using the reflection coefficient defined by Eq. (2). The main aim of the discussed method is to fit the temporal spectrum of the reflected wave calculated on the basis of the model $\hat{S}^R(\omega, \theta, d_s)$ to the spectrum of the reflected wave measured experimentally $S^R(\omega, \theta, d_s)$. To this end, the so-called cost function is defined as the least square error between the measured and simulated temporal spectra:

$$E(\omega, \theta, d_s) \equiv e(\omega, \theta, d_s)e(\omega, \theta, d_s)^T = \sum_k |e(\omega_k, \theta, d_s)|^2, \quad (6)$$

where summation is over all frequency samples (a discrete temporal spectrum is assumed here). In Eq. (6, 7), $\theta = \{\alpha_s, \alpha_p, \rho_s, \rho_p, \rho_w, c_s, c_p, c_w\}$ denotes the vector of the system parameters which are assumed to be known. Minimizing the cost function allows us to determine the value of layer thickness d_s which best fits the relevant measurements and provides the desired solution.

2. MATERIALS AND METHODS

The developed method was tested using experimental data obtained from the custom design model that consisted of a solid thin layer glued to the porous material shown in Fig. 2. The layer material (Sawbones, Pacific Research Laboratory Inc, Vashon, WA) was made of oriented glass-fibers mixed with epoxy. The material is transversely isotropic, with elastic properties close to those of real bones. The attenuation coefficient of the layer material was $\alpha_s = 2.6$ dB/cm, as reported in [7]. The longitudinal wave velocity c_s measured with the pulse echo method at a center frequency of 6 MHz, was equal 2900 m/s. The frequency of 6 MHz was chosen to obtain the separation of the pulses reflected from the bottom surfaces of the plate. The solid plate was bonded to a porous material with a rigid polyurethane foam core and with a thickness of about 30 mm, which models the cancellous bone [8], as illustrated in Fig. 2. Both the plate and porous material were immersed in water. To simplify the applied model (Eq. 1-4), the attenuation of the water was neglected. To simplify the analysis, the acoustic wave velocities c_s and c_p were assumed to be constant, taking their values measured at certain reference frequencies. For the attenuation coefficients in the solid layer and porous regions the following frequency dependence was assumed [9]:

$$\alpha_i(\omega) = \alpha_i(\omega_0) \left(\frac{\omega}{\omega_0} \right)^{n_i}, \quad i = s, p, \quad (7)$$

where $\alpha_i(\omega_0)$ is the attenuation coefficient at reference frequency ω_0 ; n_i – the certain empirical constant, chosen from in the range (1 – 2).



Fig. 2. The sample used in experiments.

The mass density of the foam ρ_f , equal to 1200 kg/m^3 , was considered [8]. The longitudinal wave velocity c_p , from the porous material sample as well as the corresponding attenuation coefficient α_p , were measured with the pulse echo method at a center frequency of 0.6 MHz. The frequency of 0.6 MHz was chosen because of the high attenuation (see Table 1) of the porous material and the thickness of the sample (approximately 30 mm). The main parameters of the custom design model used in these experiments are referenced in Table 1.

Table. 1. Material properties of the custom design model.

d_s , mm	c_s , m/s	α_s , dB/cm at 1 MHz	ρ_s , kg/m^3	c_p , m/s	α_p , dB/cm at 0.5 MHz	ρ_f , kg/m^3	ρ_p , kg/m^3
1.05	2900	2.6	1640	1641	10.8	1200	1457

The thickness of the solid layer sample was measured with a digital caliper. The corresponding density of the foam ρ_p was computed using the following equation:

$$\rho_p = P\rho_w + (1 - P)\rho_f, \quad (8)$$

where the mass density of the water was $\rho_w = 1000 \text{ kg/m}^3$ and P was the porosity of the foam which was measured and was equal to 0.88 (88%). The pulse-echo method was used in the experimental verification of the developed method. To this end, a flat transducer of 25 mm in diameter excited by a sine cycle of 600 kHz was used. The transmit pulse was obtained using a pulse generator (the Tektronix AFG 3252 dual channel arbitrary function generator). The reflected signal was detected using the same transducers. The radio frequency (RF) data collected on each measurement point was first amplified using a high power pulse amplifier and then recorded by a digital storage oscilloscope (model DSO9104A, Keysight Technologies Inc.) at a 400 MHz temporal sampling rate and transferred to a PC for further off-line processing in Matlab[®] in order to test the developed method. To solve the optimization problem, that is to say the minimizing of the cost function in Eq. (6), the simulated annealing algorithm implemented in the *simulannealbnd* function from the Matlab[®] package 'Optimization Toolbox', was used. This method is based on the comparison of the temporal spectra of measured and simulated reflected signals, Eq. (6). In the numerical simulations, the corresponding temporal spectra were truncated at an upper frequency of 1.25 MHz. Five measurements were taken at spatial positions 5 mm apart. At each measurement point the optimization using the simulated annealing was repeated $N=50$ and the mean values of \bar{d}_s were evaluated. Then the obtained values were averaged yielding the final estimate of thickness d_s . This value was further compared with the reference values shown in Table 1.

3. RESULTS AND DISCUSSION

The results of the simulations performed in Matlab[®] are presented in Table 2.

Table 2. Measured values and relative errors of the thickness of the solid layer fixed to the porous material.

measurement	\bar{d}_s , mm	d_s , mm	\hat{d}_s , mm	δ_d , %
#1	1.0418	1.0651	1.05	1.44
#2	1.0659			
#3	1.0783			
#4	1.0753			
#5	1.0641			

In Table 2, \hat{d}_s denotes the reference value of the layer thickness from Table 1; δ_d being the corresponding relative error:

$$\delta_d = \frac{d_s - \hat{d}_s}{\hat{d}_s} \cdot 100\%, \quad (9)$$

In Fig. 3, the results summarized in Table 2 are illustrated in graphical form, presenting the estimated mean values of the layer thickness.

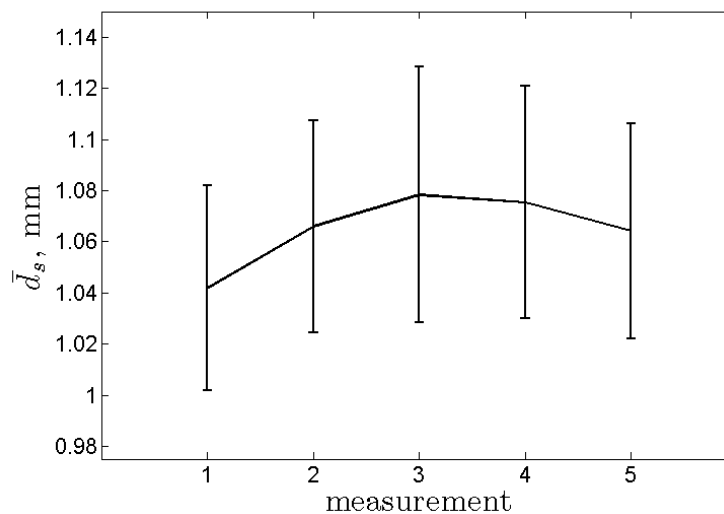


Fig. 3. The mean values \bar{d}_s and the standard deviations σ_d , of the layer thickness for $N=50$ estimations at each measurement.

The error bars show standard deviations σ_d estimated from 50 measurements at each spatial point spaced 5 mm apart along the custom design model. As can be seen from Table 2, the relative error of layer thickness evaluation was 1.44%. This proves that the developed method is promising for further study and development. Specifically, it is important to point out that in the presented method the acoustic wave speed in the solid layer was known. In real situations, c_s is usually unknown. Therefore, further research will be focused on a generalization of the discussed method for the case of the simultaneous estimation of the layer thickness and acoustic (longitudinal) wave velocity in a layer.

This method may be of potential use in the estimation of the thickness of a cortical bone layer. The influence of cortical bone thickness can substantially reduce the accuracy of Broadband

Ultrasound Attenuation (BUA) measurements from the cancellous bone area, which is a main indicator of bone disease, such as osteoporosis [10-13]. Therefore, for the reliable assessment of trabecular bone quality, it is necessary to take cortical bone thickness into account. This can be achieved only once the thickness of the cortical bone layer is known.

REFERENCES

- [1] J. Karjalainen, O. Riekkinen, J. Toyras, H. Kroger, J. Jurvelin, Ultrasonic Assessment of Cortical Bone Thickness In Vitro and In Vivo, *IEEE Transactions on Ultrasonics, Ferroelectrics, and Frequency Control*, Vol. 55, 2008.
- [2] J. Karjalainen, Novel Pulse-Echo Ultrasound Methods for Diagnostics of Osteoporosis, Phd thesis, University of Eastern Finland, 2011.
- [3] K. Falińska, J. Litniewski, J. Tasinkiewicz, Assesment of cortical bone thickness using cepstrum analysis. Simulation study, *Hydroacoustics*, 17, 47 – 56, 2014.
- [4] F. Hagglund, J. Martinsson, J.E. Carlson, C. Carlander, Model-Based Characterization of Thin Layers Using Pulse-Echo, *Ultrasound Proceedings of the International Congress on Ultrasonics (Paper ID 1562, Session R17: NDT Modeling and Simulation)*, Vienna 2007.
- [5] A. Briggs, O. Kolosov, *Acoustic Microscopy*, Oxford University Press, New York 2010.
- [6] P.R. Stepanishen, Reflection and transmission of acoustic wideband plane waves by layered viscoelastic media, *J. Acoust. Soc. Am.* 71(1), 9 – 21, 1982.
- [7] J.G. Minonzio, J. Foiret, M. Talmant, P. Laugier, Impact attenuation on guided mode wavenumber measurement in axial transmission on bone mimicking plates, *J. Acoust. Soc. Am.* 130(6), 3574 – 3582, 2011.
- [8] <http://www.matweb.com/search/GetMatlsByManufacturer.aspx?manID=191>.
- [9] A. Nowicki, *Principles of Doppler Ultrasound*, p. 37, PWN, Warsaw, 1995 (in Polish).
- [10] Xia Y, Lin W, Qin Y X, The influence of cortical end-plate on broadband ultrasound attenuation measurements at the human calcaneus using scanning confocal ultrasound, *J. Acoust. Soc. Am.* 118 (3), Pt. 1, September 2005.
- [11] C.M. Langton, M. Subhan, Computer and experimental simulation of a cortical end-plate phase cancellation artefact in the measurement of BUA at the calcaneus, *Physiol Meas.* 2001 Aug; 22(3):581-7.
- [12] C.M. Langton, C.F. Njeh, R. Hodgkinson, J.D. Currey, Prediction of mechanical properties of the human calcaneus by broadband ultrasonic attenuation, *Bone* 1996 Jun;18(6):495-503.
- [13] K.A. Wear, The effect of phase cancellation on estimates of calcaneal broadband ultrasound attenuation in vivo, *IEEE Trans Ultrason Ferroelectr Freq Control.* 2007 Jul;54(7):1352-9.